



When product integrity counts...


Manufacturers of laboratory calibrated temperature and humidity data loggers, real-time monitoring and cold chain solutions

Optional Calibration Expiry Feature

The recalibration time is usually stipulated by the User's standard operating procedures, e.g., 2 years.

The Calibration Expiry feature is built in to the loggers during manufacture (it is not software activated) and therefore needs to be requested at the time of placing the order, and confirmed in writing.

On Accessing Logger:

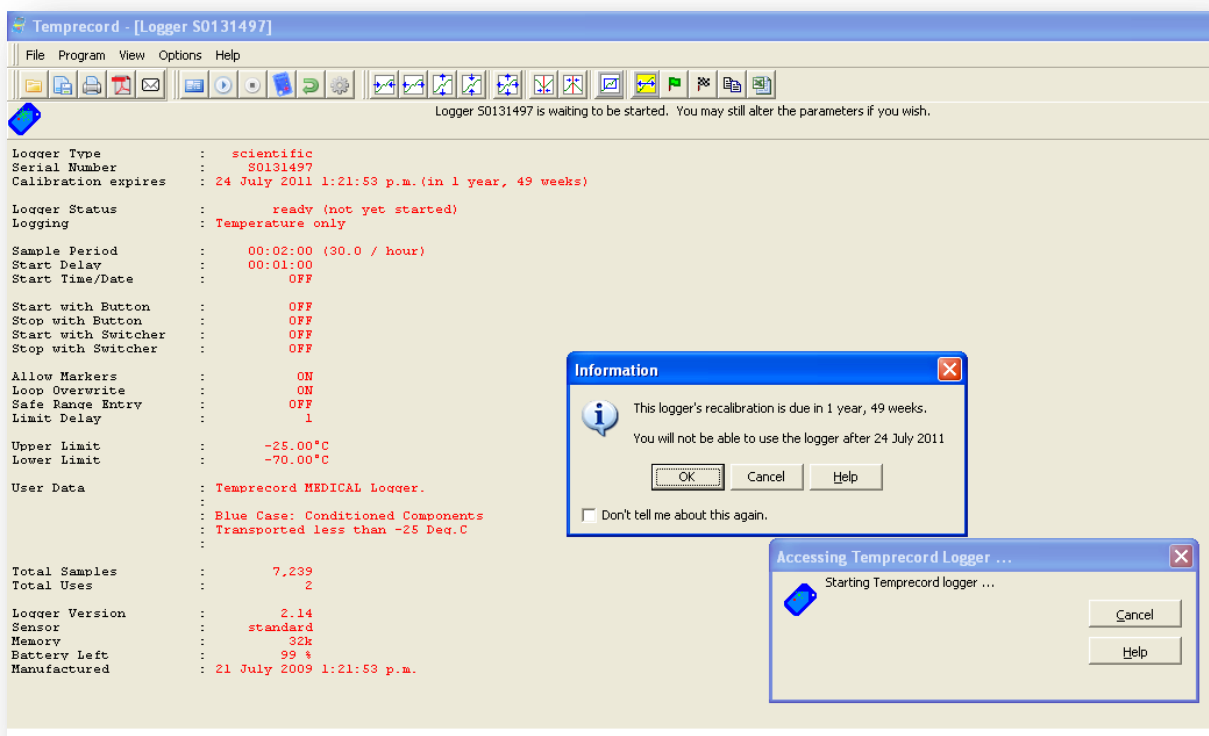


The "Information" message above will show every time a logger is accessed but can be deactivated by selecting the tab **Options/General** and unselecting "Prompt on loggers with calibration".

Built in to the software is a "warning" message that will appear 3 weeks before recalibration is due and this message cannot be deactivated. This is shown in a later screen...

Optional Calibration Expiry Feature


At 3 weeks before expiry of calibration period:

A “warning” message will appear 3 weeks before the calibration period expires and *this cannot be deactivated*. See image below.

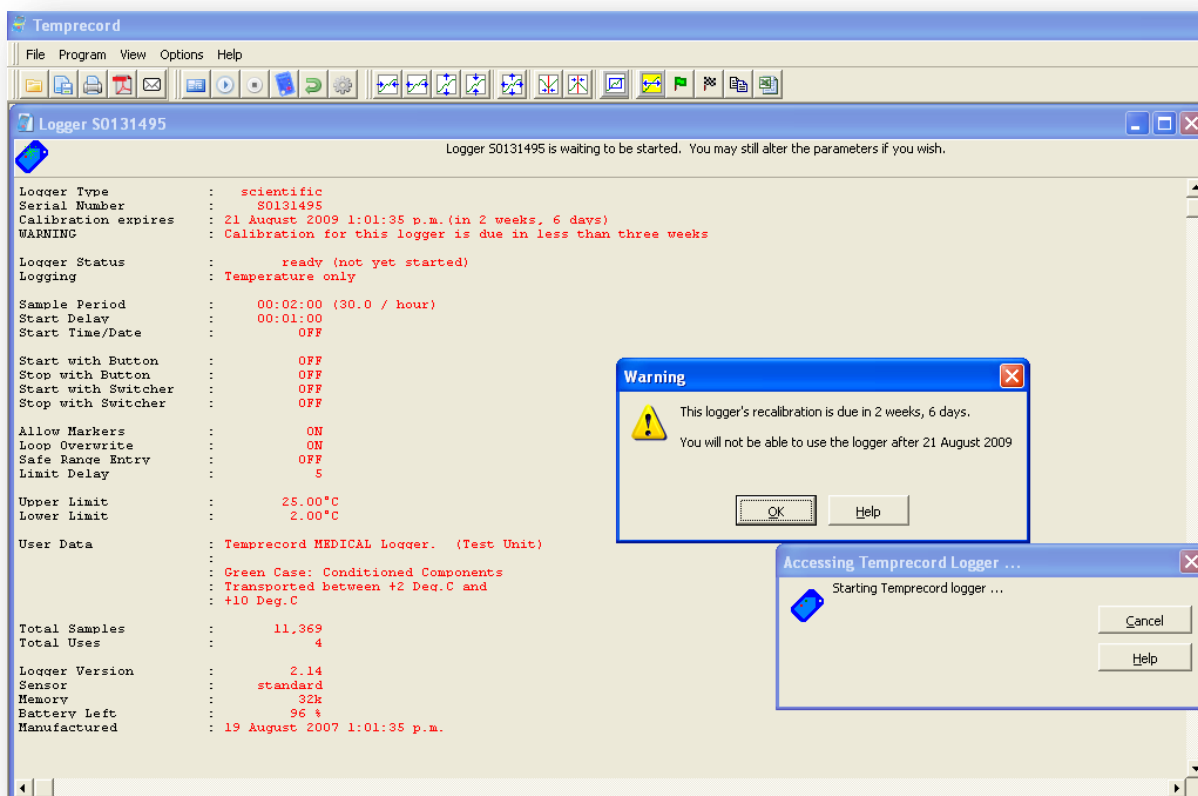

Optional Calibration Expiry Feature

Calibration Period Expired:

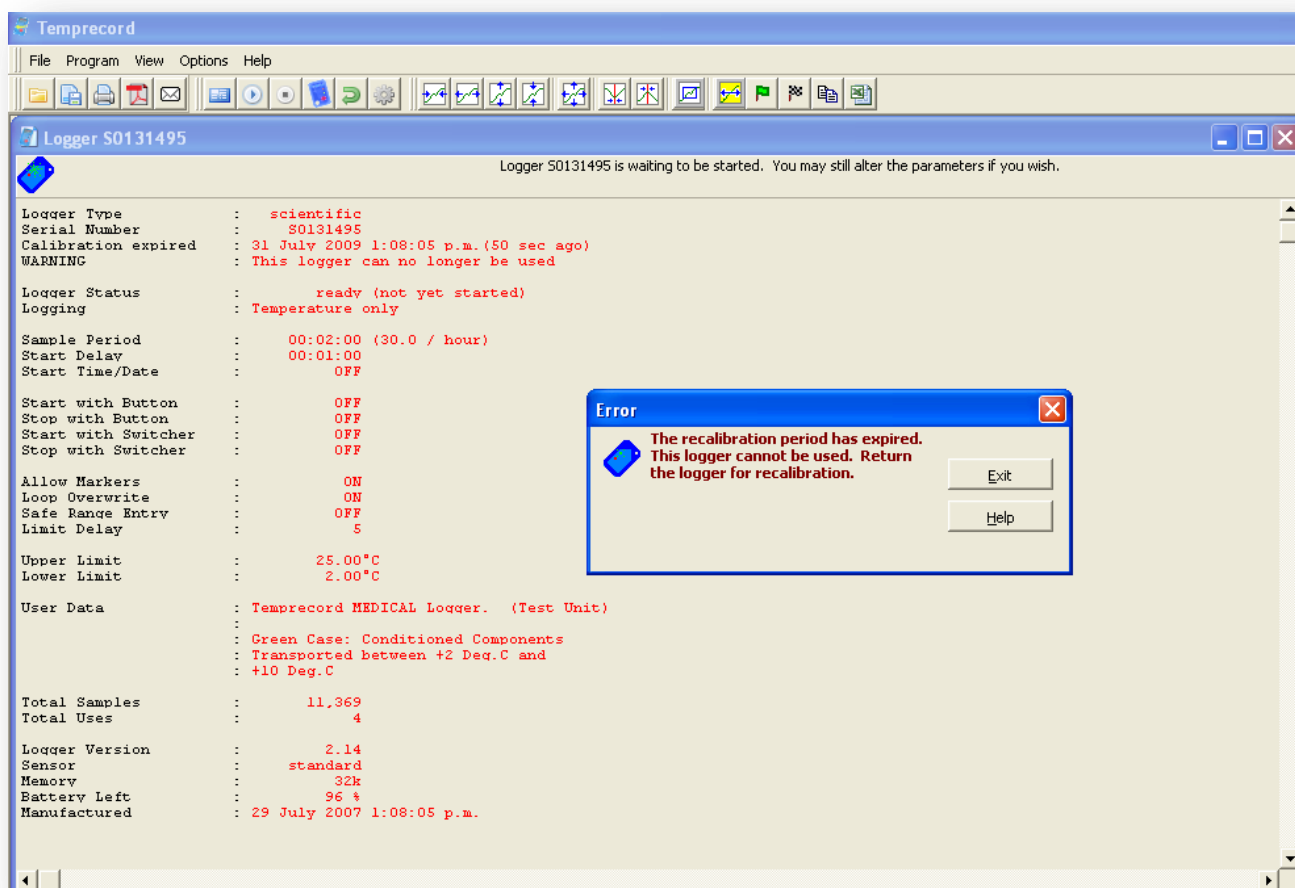

The above message will appear once the calibration period has expired and it cannot be reused again until recalibrated.

If the logger calibration period expires while the logger is on a journey, it will continue to log and store the data until full or stopped, but cannot be reused until recalibrated.